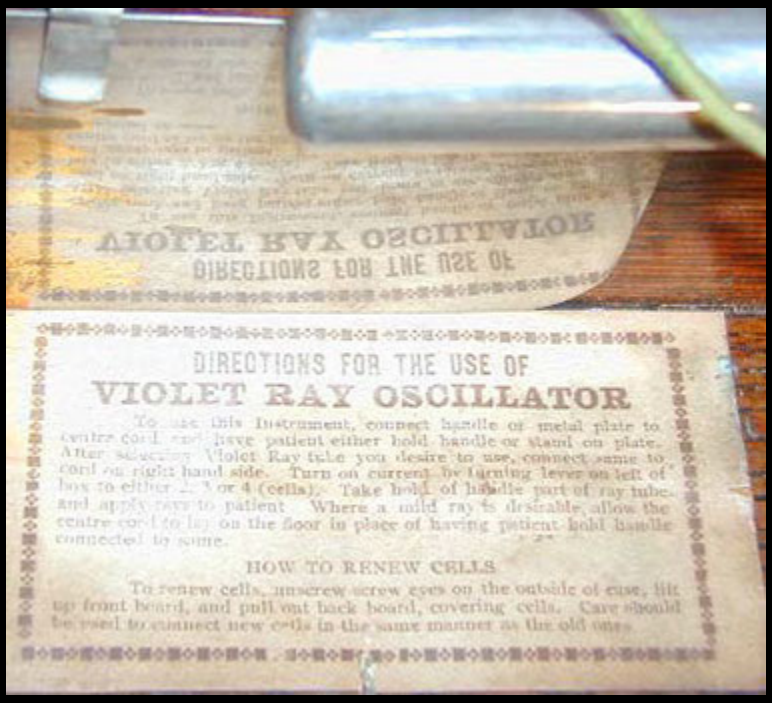

DIRECTIONS FOR THE USE OF

VIOLET RAY OSCILLATOR

To use this Instrument, connect handle or metal plate to centre cord and have patient either hold handle or stand on plate. After selecting Violet Ray tube you desire to use, connect same to cord on right hand side. Turn on current by turning lever on left of box to either 2, 3 or 4 (cells). Take hold of handle part of ray tube and apply rays to patient. Where a mild ray is desirable, allow the centre cord to lay on the floor in place of having patient hold handle connected to same.

HOW TO RENEW CELLS

To renew cells, unscrew screw eyes on the outside of case, lift up front board, and pull out back board, covering cells. Care should be used to connect new cells in the same manner as the old ones.

(C) Jeff Behary 2021